



Ethyl Glucuronide (EtG) Urine Test Panel

Catalogue No. See Box label

The T-Dip® Ethyl Glucuronide (EtG) Urine Test Panel is a competitive binding, lateral flow immunochromatographic assay for qualitative and simultaneous detection of Ethyl Glucuronide (EtG) in human urine with below cutoff concentration and approximate detection time:

Drug (Identifier)	Calibrator	Cut-off Level	Minimum Detection Time	Maximum Detection Time
Ethyl Glucuronide (EtG)	Ethyl Glucuronide	300 ng/mL	1-2 hours	Up to 3+ days

It is intended for forensic use only.

The test is not intended to distinguish between prescription use or abuse of these drugs. Clinical consideration and professional judgment should be applied to any drug of abuse test result, particularly in evaluating a preliminary positive result.

The test provides only preliminary test results. To obtain a confirmed analytical result, a more specific alternate chemical method must be used. Chromatography/Mass Spectrometry (GC/MS) or Liquid Chromatography/Tandem Mass Spectrometry (LC/MS-MS) is the recommended confirmatory method.

WARNINGS AND PRECAUTIONS

1. The test kit is for external use only. Do not swallow.
2. Discard after first use. The test kit cannot be used more than once.
3. Do not use the test kit beyond expiration date.
4. Do not use the test kit if the pouch is punctured or not sealed.
5. Keep out of the reach of children.
6. Do not read after 5 minutes.

CONTENT OF THE KIT

1. Test devices, one test in one pouch. One pouch containing a test and a desiccant. The desiccant is for storage purposes only, and is not used in the test procedures.
2. Package Insert

MATERIAL REQUIRED BUT NOT PROVIDED

1. Urine collection cup
2. Timer or clock

STORAGE AND STABILITY

Store at 4°C-30°C (39°F-86°F) in the sealed pouch up to the expiration date. Keep away from direct sunlight, moisture and heat. DO NOT FREEZE.

SPECIMEN COLLECTION

WHEN TO COLLECT URINE FOR THE TEST?

The minimum detection time of Ethyl Glucuronide (EtG) is 1-2 hours, urine specimens may be collected 1-2 hours after the suspected drug use.

HOW TO COLLECT URINE?


Instruct the donor to void directly into the urine collection cup. Wipe off any splashes or spills

that may be on the outside of the cup. It is recommended to wear gloves when handling the urine collection cup with urine specimen.

TEST PROCEDURE

Test should be performed at room temperature 18°C-30°C (65°F-86°F).

1. Remove the test device from the foil pouch by tearing at the notch. Use it as soon as possible.
2. Hold one side of the device with one hand. Use the other hand to pull out the cap and expose the absorbent end.
3. Immerse the absorbent end into the urine specimen for approximately 10 seconds. **Make sure that the urine level is not above the marked line printed on the front of the device.**
4. Re-cap the device and lay it flat on a clean, dry, non-absorbent surface.
5. Read the result at 5 minutes. **Do not read after 5 minutes.**



Note: Results after more than 5 minutes may be not accurate and should not be read.

READING THE RESULTS

Negative (-)

A colored band is visible in each Control Region (C) and the appropriate Test Region (T). It indicates that the concentration of the corresponding drug of that specific test zone is zero or below the detection limit of the test.

Preliminary Positive (+)


A colored band is visible in each Control Region (C). No colored band appears in the appropriate Test Region (T). It indicates a preliminary positive result for the corresponding drug of that specific test zone.

Invalid

If a colored band is not visible in each of the Control Region (C) or a colored band is only visible in each of the Test Region (T), the test is invalid. Another test should be run to re-evaluate the specimen. If test still fails, please contact the distributor with the lot number.

Note: There is no meaning attributed to line color intensity or width.

The preliminary positive test result does not always mean that a person took illegal drugs. The negative test result does not always mean that a person did not take illegal drugs. There could be a number of factors that affect the reliability of drug tests.

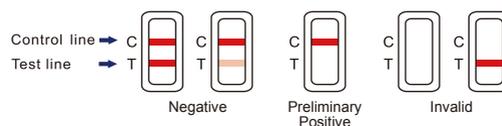

What is the False Positive Test?

The definition of the false positive test would be an instance where a substance is identified incorrectly by the T-Dip® Ethyl Glucuronide (EtG) Urine Test Panel. The most common causes of the false positive test are cross reactants. Certain foods and medicines, diet plan

drugs and nutritional supplements may cause the false positive test result.

What Is the False Negative Test?

The definition of the false negative test is that the initial drug is present but isn't detected by the T-Dip® Ethyl Glucuronide (EtG) Urine Test Panel. If the specimen is diluted, or the specimen is adulterated that may cause false negative result.

If suspect someone is taking drugs but get the negative test results, please test again at another time.

TEST LIMITATIONS

1. This test kit has been developed for testing urine samples only. No other fluids have been evaluated. DO NOT use it to test anything other than urine.
2. Adulterated urine samples may produce false results. Strong oxidizing agents such as bleach (hypochlorite) can oxidize drug analytes. If a specimen is suspected of being adulterated, obtain a new specimen.
3. It is possible that technical or procedural errors, as well as other interfering substances in the urine specimen may cause false results.
4. This test is a qualitative screening assay. It is not designed to determine the quantitative concentration of drug or the level of intoxication.

SUMMARY

Ethyl Glucuronide is a direct metabolite of alcohol. Presence in urine may be used to detect recent alcohol intake, even after alcohol is no longer measurable. Traditional laboratory methods detect the actual alcohol in the body, which reflects current intake within the past few hours (depending on how much was consumed). The presence of EtG in urine is a definitive indicator that it can be detected in the urine for 3 to 4 days after drinking alcohol even alcohol is eliminated from the body. Therefore, EtG is a more accurate indicator of the recent intake of alcohol than measuring for the presence of alcohol itself. The EtG test can aid in the diagnosis of drunk driving and alcoholism, which has important significance in the forensic identification and medical examination.

PRINCIPLE

The T-Dip® Ethyl Glucuronide (EtG) Urine Test Panel is a competitive immunoassay that is used to screen for the presence of drugs in urine. It is chromatographic absorbent device in which drugs in a specimen competitively combined to a limited number of drug monoclonal antibody (mouse) conjugate binding sites.

When the absorbent end is immersed into urine specimen, the urine is absorbed into the device by capillary action, mixes with the respective drug monoclonal antibody conjugate, and flows across the pre-coated membrane. When sample drug levels are zero or below the target cutoff (the detection sensitivity of the test), respective drug monoclonal antibody conjugate binds to the respective drug-protein conjugate immobilized in the Test Region (T) of the device. This produces a colored Test line that, regardless of its intensity, indicates a negative result.

When sample drug levels are at or above the target cutoff, the free drug in the sample binds to the respective drug monoclonal antibody conjugate preventing the respective drug monoclonal antibody conjugate from binding to the respective drug-protein conjugate immobilized in the Test Region (T) of the device. This prevents the development of a distinct colored band in the Test Region (T), indicating a potentially positive result.

To serve as a procedure control, a colored line will appear at the Control Region (C), if the test has been performed properly. This control line should always appear regardless of the presence of drug or metabolite. If the control line does not appear the test device should be discarded.

QUALITY CONTROL

Users should follow the appropriate federal, state, and local guidelines concerning the frequency of assaying external quality control materials. Even though there is an internal procedural control line in the test device in the Control Region (C), the use of external

controls is strongly recommended as good laboratory testing practice to confirm the test procedure and to verify proper test performance. Positive and negative controls should give the expected results. When testing the positive and negative controls, the same assay procedure should be adopted. External Control (positive and negative) should be run with each new lot of test received, each new shipment, each new operator and monthly to determine that tests are working properly.

PERFORMANCE CHARACTERISTICS

Accuracy

Eighty clinical urine specimens were analyzed by GC/MS or LC-MS/MS and by the T-Dip® Ethyl Glucuronide (EtG) Urine Test Panel. Each test was read by three viewers. Samples were divided by concentration into five categories: Drug Free, Less than Half the Cutoff, Near Cutoff Negative, Near Cutoff Positive, and High Positive. Results were as follows:

Result	Drug Free	Less than Half the Cutoff	Near Cutoff Negative (Between 50% below the cutoff and the cutoff)	Near Cutoff Positive (Between the cutoff and 50% above the cutoff)	High Positive (Greater than 50% above the cutoff)	% Agreement with GC/MS or LC/MS	
Viewer A	+	0	0	0	17	21	95%
	-	10	12	18	2	0	100%
Viewer B	+	0	0	0	18	21	97.5%
	-	10	12	18	1	0	100%
Viewer C	+	0	0	0	18	21	97.5%
	-	10	12	18	1	0	100%

Precision and Sensitivity

To investigate the precision and sensitivity, each drug sample was analyzed at the following concentrations: cutoff -100%, cutoff -75%, cutoff -50%, cutoff -25%, cutoff, cutoff +25%, cutoff +50%, cutoff +75% and the cutoff +100%. All concentrations were confirmed with GC/MS or LC-MS/MS. The study was used three different lots of the T-Dip® Ethyl Glucuronide (EtG) Urine Test Panel. The data are summarized below:

Approximate Concentration of Sample (ng/mL)	Number of Determinations per Lot	Results (Negative/Positive)		
		Lot 1	Lot 2	Lot 3
0	50	50/0	50/0	50/0
75	50	50/0	50/0	50/0
150	50	50/0	50/0	50/0
225	50	50/0	50/0	50/0
300	50	5/45	4/46	5/45
375	50	0/50	0/50	0/50
450	50	0/50	0/50	0/50
525	50	0/50	0/50	0/50
600	50	0/50	0/50	0/50

Specificity and Cross Reactivity

To test the specificity of the test, the test device was used to test various drugs, drug metabolites and other components of the same class that are likely to be present in urine. All the components were added to drug-free normal human urine. The following structurally related compounds produced positive results with the test when tested at levels equal to or greater than the concentrations listed below.

Substance	Concentration (ng/mL)
Ethyl Glucuronide (EtG)	
Ethyl Glucuronide	300

Effect of Urinary Specific Gravity

The results demonstrate that the urinary specific gravity range of 1.000-1.035 does not affect the test results.

Effect of Urinary pH

The results demonstrate that the range of urinary pH from 4 to 9 does not interfere with the performance of test.

Interfering Substances

The following compounds were added to drug-free urine, urine with drug concentration 25% below the cutoff, and urine with drug concentration 25% above the cutoff for the corresponding T-Dip® Ethyl Glucuronide (EtG) Urine Test Panel. All potential interferents were added at a concentration of 100 µg/mL. None of the urine samples showed any deviation from the expected results.

Acetaminophen	Fluoxetine HCl	Olanzapine
Acid Reducer	Fluvoxamine	Omeprazole
Acyclovir	Gabapentin	Paliperidone
Amiodarone HCl	Gilbenclamide	Papaverine
Amlodipine Mesylate	Gliclazide	Paroxetine
Amoxicillin	Glipizide	Penfluridol
Ampicillin	Glucose	Penicillin V Potassium
Aripiprazole	Haloperidol	Pethidine HCl
Aspirin	Heartburn Relief	Pioglitazone HCl
Atorvastatin Calcium	Hydrochlorothiazide	Piracetam
Atropine	Ibuprofen	Pravastatin Sodium
Captopril	Isosorbide Esters	Prednisone Acetate
Carbamazepine	Ketoconazole	Propranolol HCl
Cefaclor	Lamotrigine	Propylthiouracil
Cephalexin	Lansoprazole	Pseudoephedrine HCl
Cephadrine	Levofloxacin	Quetiapine
Ciprofloxacin HCl	Levonorgestrel	Ranitidine HCl
Clarithromycin	Levothyroxine Sodium	Rifampicin
Clopidogrel Bisulfate	Lidocaine HCl	Risperidone
Clozapine	Lisinopril	Sertraline HCl
Cortisone	Lithium Carbonate	Sildenafil Citrate
Dextromethorphan HBr	Loratadine	Simvastatin
Diclofenac	Magnesium	Spironolactone
Digoxin	Metoprolol Tartrate	Tetracycline
Diphenoxylate HCl	Mifepristone	Topiramate
Dirithromycin	Mirtazapine	Trazodone HCl
Domperidone	Montelukast Sodium	Triamterene
Duloxetine	Mosapride	Valproate
Enalapril Maleate	Nifedipine	Venlafaxine HCl
Epinephrine HCl	Nikethamide	Vitamin B1
Esomeprazole Magnesium	Nimodipine	Vitamin B2
Estrogen	Naproxen sodium	Vitamin C
Diphenhydramine	Nitroglycerin	
Fenofibrat	Noscapine	

ASSISTANCE

If you have any question regarding to the use of this product, please call our Toll Free Number 1-888-444-3657 (9:30 a.m. to 5:00 p.m. CDT M-F).

BIBLIOGRAPHY OF SUGGESTED READING

Baselt, R.C. Disposition of Toxic Drugs and Chemicals in Man. Biomedical Publications, Davis, CA, 1982.
 Ellenhorn, M.J. and Barceloux, D. G Medical Toxicology. Elsevier Science Publishing Company, Inc., New York, 1988.
 Gilman, A. G., and Goodman, L. S. The Pharmacological Fluids, in Martin WR (ed): Drug Addiction I, New York, Spring – Verlag, 1977.

Harvey, R.A., Champe, P.C. Lippincotts Illustrated Reviews. Pharmacology. 91-95, 1992.
 Hawwks RL, CN Chiang. Urine Testing for drugs of Abuse. National Institute for Drug Abuse (NIDA), Research Monography 73, 1986.
 Hofmann F.E., A Handbook on Drug and Alcohol Abuse: The Biomedical Aspects, New York, Oxford University Press, 1983.
 McBay, A. J. Clin. Chem. 33,33B-40B, 1987.

ADDITIONAL INFORMATION AND RESOURCES

The following list of organizations may be helpful to you for counseling support and resources. These groups also have an Internet address which can be accessed for additional information.
 National Clearinghouse for Alcohol and Drug Information www.health.org 1-800-729-6686
 Center for Substance Abuse Treatment www.health.org 1-800-662-HELP
 The National Council on Alcoholism and Drug Dependence www.ncadd.org 1-800-NCA-CALL
 American Council for Drug Education (ACDE) www.acde.org 1-800-488-DRUG

INDEX OF SYMBOLS

	Keep away from sunlight
	Store between 4°C - 30°C (39°F - 86°F)
	Keep dry
	Do not re-use

Manufactured by Guangzhou Wondfo Biotech Co., LTD
 No.8 Lizhishan Road, Science City, Luogang District
 Guangzhou, Guangdong, P.R. China 510663

Made in China

Rev. A1
 Rel.: 2019/10/24